


Research Article

6 Open Access



Electron Beams Commissioning and Initial Measurements on an Elekta Synergy Platform Linear Accelerator

Abdurraouf. M. Aghila^{1*}, Saad. S. Saad², Faraj A. Elmasrub³

***Corresponding author:**
ab.aghila@uot.edu.ly, Department of Physics, Faculty of Education, University of Tripoli, Libya.

Second Author: saadmad-di@yahoo.com, Higher Institute of Medical Sciences and Technology, Abu-Salim, Tripoli, Libya.

Third Author:
f_masrub@hotmail.com, National Cancer Institute of Sabratha, Sabratha, Libya

Received:
03 February 2023

Accepted:
26 April 2023

Publish online:
31 December 2023

Abstract

A linear accelerator (Linac) must be commissioned for use in treating cancer patients. This research work aims to analyze part of the electron beam data produced by the Elekta Synergy Platform Linac at the radiotherapy department at Tripoli University Hospital, Tripoli, Libya. In this paper, percentage depth dose (PDD), beam profile and applicators factor were studied at five different electron beam energies (4, 6, 8, 10 and 12 MeV). The relative measurement part of this study was carried out using a PTW MP3-M 3D water scanning system, and the absolute measurement was taken using a plane parallel ionization chamber and a unidose E electrometer. The analysis for these measurements has yielded the following results: a) The Penetrative qualities of all the electron beam energies were within the manufacturer's tolerance limits of $\pm 1\%$; b) the maximum values of beam flatness of 2.94 and beam symmetry of 1.93 are within the accepted limits of International Electrotechnical Commission criteria; c) A penumbra maximum value of 1.30 was measured at the 4-MeV electron beam energy and using a $14 \times 14 \text{ cm}^2$ applicator size. All the obtained parameters were within the permissible limits. Therefore, the electron beams can be safely used for clinical purposes.

Keywords: Elekta Synergy Platform; Electron Beam Commissioning; PDD; Beam Profile; Applicator Factor.

INTRODUCTION

One common treatment method for cancer disease is radiotherapy. It uses high-energy radiation of different ionization types to destroy tumor cells. The type of treatment radiation depends on tumor size and location, tumor type, and tumor stage. For superficial tumors, electron beams are widely used due to their sharp dose fall-off and relatively short range of particles in tissue (Arunkumar et al., 2010). A linear accelerator is the most common and most sophisticated machine used for external beam radiotherapy made by different manufacturers. Linacs of different manufacturers have different structure order and design especially in Linacs treatment head. The differences in the treatment head affect the characteristics of electron and photon beams. Moreover, Linacs of the same manufacturer are slightly different in their beam characteristics (Brahme et al., 1976; Khan, 1991; IEC, 1984; Varatharaj et al., 2016).



*The Author(s) 2023. * This article is distributed under the terms of the *Creative Commons Attribution-NonCommercial 4.0 International License* (<http://creativecommons.org/licenses/by-nc/4.0/>) (<http://creativecommons.org/licenses/by-nc/4.0/>)), which permits unrestricted use, distribution, and reproduction in any medium, *for non-commercial purposes only*, provided you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons license, and indicate if changes were made.

Accurate data measurements of photon and electron beam characteristics produced by Linac, which need to be transferred into the Treatment Planning System (TPS) to predicate the radiation dose distribution inside the patient, are important factors that affect the success of radiation therapy (Acqah *et al.*, 2014). According to the recommendations of the American Association of Physicists in Medicine (AAPM) in the Task Group 40, and International Commission on Radiation Units and Measurements in report 50 (Kutcher *et al.*, 1994; ICRU, 1993), the dose delivery to tumor should be within $\pm 5\%$ of a prescribed dose. Therefore, commissioning and acceptance tests of the linear accelerator are required before setting the machine in clinical-use (Khan, 2010; Sahool *et al.*, 2012).

Due to the lack of local standards of measurement, this paper aims to present and analyze part of electron beams commissioning to allow physicists of other institutes to compare their results with those of this study. The measurements include the percentage depth dose curves, beam profiles parameters and applicators factor of an Elekta Synergy platform linear accelerator released by Elekta Oncology Systems, Crawley, UK.

MATERIALS AND METHODS

This work was carried out at Radiotherapy Department, Tripoli University Hospital in Tripoli, Libya. Measurements of percentage depth dose (PDD), beam profile and applicators factor were carried out for electron beam of nominal energies 4, 6, 8, 10 and 12 MeV generated by Elekta Synergy platform linear accelerator. The dosimetry system for measurements of PDD and beam profile was a PTW MP3-M 3D water scanning system (PTW, Freiburg, Germany). The system consists of a water tank of inner size $59.6 \times 59.4 \times 50.25 \text{ cm}^3$, a TANDEM electrometer, a TBA control unit and two 0.125 cm^3 semiflex ionization chambers for both reference and ionization field. The measured PDD and beam profile were collected using PTW MEPHYSTO mc^2 navigation software (PTW, Freiburg) version 1.6. Applicators factors were measured in polystyrene slab phantom at depth of the maximum dose using a plane parallel ionization chamber connected to PTW Unidose E electrometer at a source to surface distance (SSD) of 100 cm.

PDD and beam profiles were measured at (SSD) of 100 cm setup and at gantry and collimator angles of 0° . The applicators used for these measurements were of size $6 \times 6 \text{ cm}^2$, $10 \times 10 \text{ cm}^2$, $14 \times 14 \text{ cm}^2$ and $20 \times 20 \text{ cm}^2$ in different depths according to the electron beam applied and taking into account the bremsstrahlung contamination in the beam. All measurements were made according to TRS-277 and TRS-398 (IAEA, 1987; IAEA, 2000).

Parameters calculated from the central axis PDD according to AAPM Task Group 25 (Gerbi *et al.*, 2009) are the mean energy \bar{E}_0 and the most probable energy $E_{p,0}$ at the water phantom surface using equations (1) and (2) respectively:

$$\bar{E}_0 = 2.33 R_{50} \quad (1)$$

$$E_{p,0} = 0.22 + 1.98 R_p + 0.0025 R_p^2 \quad (2)$$

Where R_{50} is the depth at which the dose is 50% of the maximum, and R_p is the practical range.

Another important parameter is dose gradient (G), which measures how quickly the dose decreases beyond the therapeutic range and is given by equation (3) (Gerbi *et al.*, 2006; Podgorsak, 2003)

$$G = \frac{R_p}{R_p - R_q} \quad (3)$$

Where R_q is the depth at which the tangent through the dose inflection point intersects the maximum dose level. For electron beams with mean energy of 5 MeV – 30 MeV, the lower limit of G is 2.3 (Kirby *et al.*, 1985; Jamshidi *et al.*, 1987).

Beam flatness, beam symmetry and penumbra width were calculated based on measurements of beam profiles. The IEC 60976 (IEC, 2007) criteria were followed for flatness, symmetry and penumbra width calculation.

RESULTS

Penetrative quality: The penetrative quality of the electron beam is defined as the depth of the 80% point to the maximum absorbed dose on the central beam axis. Table 1 shows the results of declared and measured electron beam penetrative quality which measured at $SSD = 100\text{ cm}$ for the applicator of size $14 \times 14\text{ cm}$.

Table (1). Declared and measured values of penetrative quality of electron beams.

Nominal energy (MeV)	Penetrative quality		Difference mm
	Declared Mm	measured mm	
4	13.30	13.55	-0.25
6	20.00	19.82	+ 0.18
8	26.70	26.32	+ 0.38
10	33.30	33.64	- 0.34
12	40.00	40.20	- 0.20

Percentage depth dose: Figure 1 illustrates the percentage depth dose curves of 4, 6, 8, 10 and 12 MeV electron beam energies for the applicator of size $10 \times 10\text{ cm}^2$ at $SSD = 100\text{ cm}$.

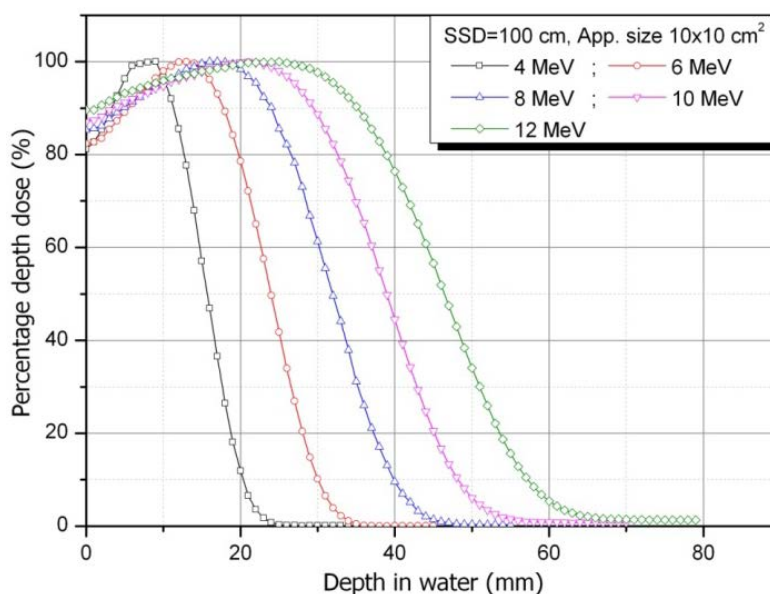


Figure (1). PDD curves of 4, 6, 8, 10 and 12 MeV electron energies for the applicator of size $10 \times 10\text{ cm}^2$ at SSD 100 cm

Electron beams parameters R_{50} , R_{80} , R_{100} , R_p , R_q , percentage surface dose D_s and bremsstrahlung contamination D_x obtained from the measured PDD at SSD of 100 cm are presented in Table 2.

Table 3 presents the calculated parameters from the measured (PDD) data for the electron beam of energies 4, 6, 8, 10 and 12 MeV and applicators of size $6 \times 6\text{ cm}^2$, $10 \times 10\text{ cm}^2$, $14 \times 14\text{ cm}^2$ and $20 \times 20\text{ cm}^2$.

Table (2). Electron beam parameters obtained from PDD at **SSD = 100 cm**.

App. Size cm ²	R ₅₀ mm	R ₈₀ mm	R ₉₀ mm	R ₁₀₀ mm	R _p mm	R _q mm	D ₂ %	D ₂ %
Electron nominal energy : 4 MeV								
6×6	16.00	12.98	11.56	8.00	20.53	11.91	79.32	0.21
10×10	15.69	12.70	11.31	8.00	19.87	11.22	81.25	0.19
14×14	16.61	13.55	12.16	9.00	20.67	12.00	80.78	0.17
20×20	16.87	13.81	12.39	9.00	21.16	12.57	81.43	0.11
Electron nominal energy : 6 MeV								
6×6	23.43	19.27	17.32	12.00	29.35	17.47	81.50	0.27
10×10	23.93	19.75	17.80	12.00	30.29	17.62	82.32	0.35
14×14	24.02	19.82	17.87	12.00	30.29	17.56	82.95	0.34
20×20	24.22	20.00	17.92	12.00	30.53	17.83	84.30	0.52
Electron nominal energy : 8 MeV								
6×6	30.69	25.82	23.24	17.00	37.63	24.09	84.62	0.61
10×10	31.91	26.54	24.03	17.00	38.57	23.77	85.27	0.38
14×14	31.73	26.32	23.74	17.00	39.86	24.35	85.49	0.71
20×20	31.72	26.33	23.76	17.00	39.48	24.48	87.04	0.52
Electron nominal energy : 10 MeV								
6×6	39.09	32.64	29.63	21.00	47.55	30.57	86.55	0.63
10×10	38.95	32.61	29.47	21.00	46.29	30.58	87.03	0.84
14×14	40.03	33.64	30.50	21.00	47.71	31.38	87.17	0.66
20×20	39.94	33.54	30.40	21.00	47.32	31.07	88.22	0.47
Electron nominal energy : 12 MeV								
6×6	46.28	38.62	34.75	25.00	56.69	35.43	89.55	1.11
10×10	46.43	38.93	35.15	25.00	56.42	35.20	89.61	1.44
14×14	47.77	40.20	36.40	25.00	56.57	36.25	89.13	1.28
20×20	47.50	39.98	36.26	25.00	55.90	36.59	90.38	1.03

Table (3). Electron beam parameters calculated by PDD at **SSD = 100 cm**.

App. Size (cm ²)	E _{p,0} (MeV)	E ₀ (MeV)	G	%error E _{p,0} & Nominal Energy
Electron nominal energy : 4 MeV				
6×6	4.19	3.73	2.38	-4.81
10×10	4.05	3.66	2.30	-1.37
14×14	4.22	3.87	2.38	-5.54
20×20	4.32	3.93	2.46	-8.09
Electron nominal energy : 6 MeV				
6×6	6.05	5.46	2.47	-0.81
10×10	6.25	5.57	2.39	-4.15
14×14	6.25	5.60	2.38	-4.15
20×20	6.30	5.64	2.40	-4.99
Electron nominal energy : 8 MeV				
6×6	7.83	7.15	2.78	2.17
10×10	8.03	7.44	2.61	-0.38
14×14	8.31	7.39	2.57	-3.89
20×20	8.23	7.39	2.63	-2.85
Electron nominal energy : 10 MeV				
6×6	10.00	9.11	2.80	-0.02
10×10	9.72	9.08	2.95	2.77
14×14	10.04	9.33	2.92	-0.38
20×20	9.95	9.31	2.91	0.49
Electron nominal energy : 12 MeV				
6×6	12.05	10.78	2.67	-0.42
10×10	11.99	10.82	2.66	0.09
14×14	12.02	11.13	2.78	-0.19
20×20	11.87	11.07	2.89	1.07

The relation between the mean energy \bar{E}_0 and R_{50} is illustrated in Figure 2.

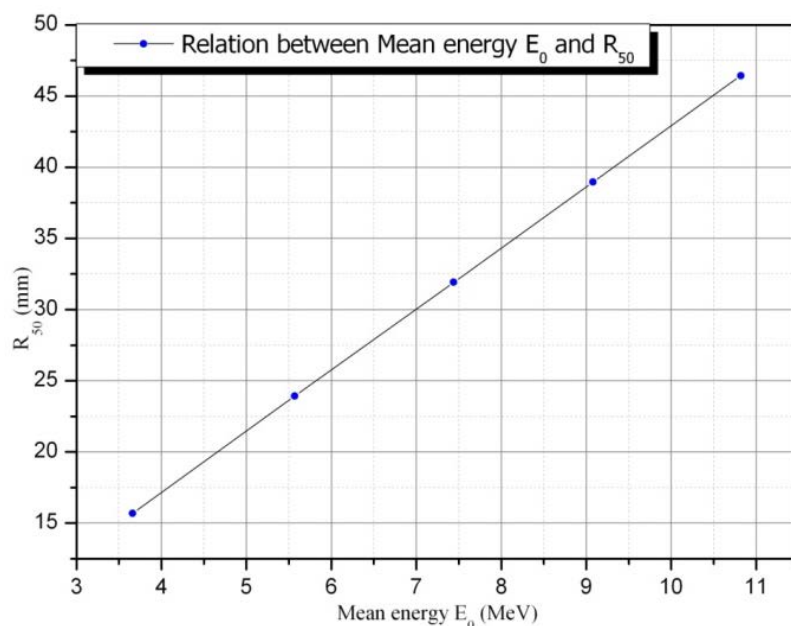


Figure (2). The relation between \bar{E}_0 and R_{50}

Beam profiles:

Figures 3, 4, 5 and 6 illustrate selected beam profiles for energies 4 MeV and applicator size 6×6 cm², 6 MeV and applicator size 10×10 cm², 10 MeV and applicator size 20×20 cm², and 12 MeV and applicator size 14×14 cm², respectively.

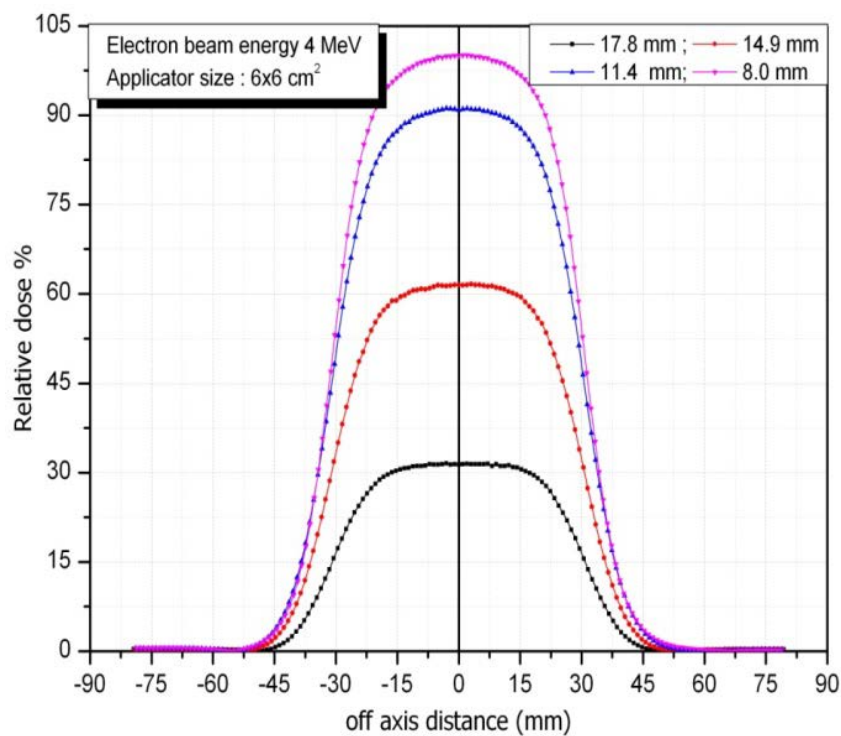


Figure (3). Beam profile for 4 MeV electron beam and applicator of size 6×6 cm²

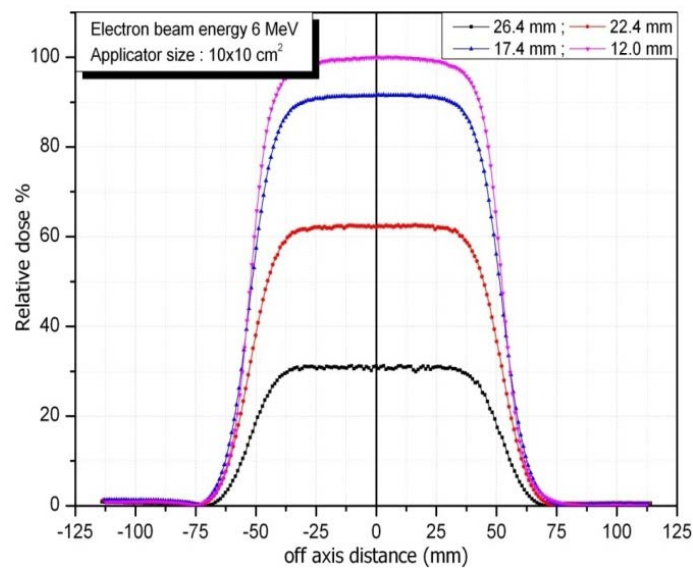


Figure (4). Beam profile for 6 MeV electron beam and applicator of size $10 \times 10 \text{ cm}^2$.

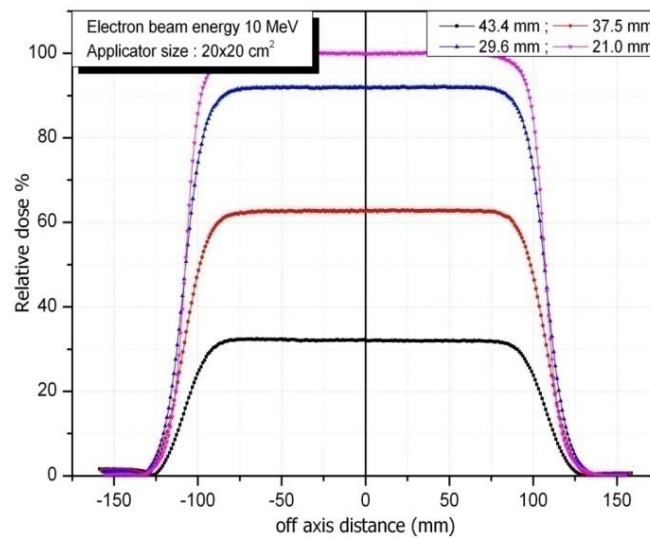


Figure (5): Beam profile for 10 MeV electron beam and applicator of size $20 \times 20 \text{ cm}^2$.

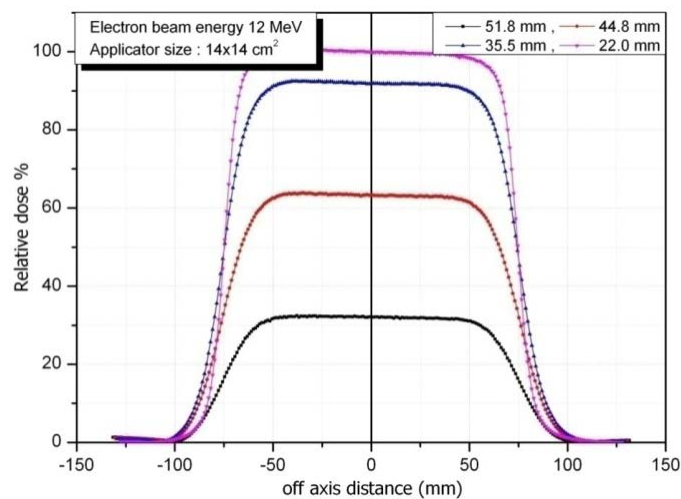


Figure (6). Beam profile for 12 MeV electron beam and applicator size $14 \times 14 \text{ cm}^2$.

The characteristics of beam profiles (beam flatness, beam symmetry and penumbra) for electron beam energies 4, 6, 8, 10 and 12 MeV using two applicators of size $14 \times 14 \text{ cm}^2$ and $20 \times 20 \text{ cm}^2$ are tabulated in Table 4.

Table (4). Beam profiles characteristics of the electron beam

App. size (cm ²)	Flatness %	Symmetry %	Penumbra width (cm)	
			L	R
Electron beam energy: 4 MeV				
14×14	2.94	1.93	1.28	1.30
20×20	2.23	0.12	1.23	1.27
Electron beam energy: 6 MeV				
14×14	2.14	0.22	1.19	1.20
20×20	1.14	1.33	1.14	1.14
Electron beam energy: 8 MeV				
14×14	2.59	0.05	1.12	1.14
20×20	1.81	0.74	1.09	1.11
Electron beam energy: 10 MeV				
14×14	2.23	1.82	1.17	1.19
20×20	1.10	0.03	1.13	1.14
Electron beam energy: 12 MeV				
14×14	2.39	0.47	1.01	1.03
20×20	1.67	1.14	0.96	0.97

Applicators factors:

Applicator factor defines the ratio of output of the utilized applicator to the output of the reference applicator ($10 \times 10 \text{ cm}^2$). Table 5 represents the applicator factors measured at the depth of dose maximum and SSD=100 cm.

Table (5). Applicators factor of energies 4, 6, 8, 10 and 12 MeV electron beams.

Applicator size (cm^2)	Electron energy (MeV)				
	4	6	8	10	12
6×6	0.847	0.934	0.956	0.976	0.984
10×10	1.000	1.000	1.000	1.000	1.000
14×14	1.041	1.013	0.987	0.977	0.982
20×20	1.036	1.018	0.994	0.965	0.976

DISCUSSION

The maximum deviation of the measured value from the declared value of penetrative quality should be $\pm 1 \text{ mm}$ as recommended by manufacturer customer acceptance tests (Elekta, 2007). The results showed that the maximum deviation was 0.37 mm, which occurred for 8 MeV nominal energy. This is within the acceptable limit of $\pm 1 \text{ mm}$. As shown in Figure 1, the measured PDD is increased with electron beam energy and is decreased with depth. The rapidness of the radiation dose is a decreasing function of electron beam energy while the magnitude of bremsstrahlung contamination is an increasing function of electron beam energy.

The bremsstrahlung contamination to the central axis percentage depth dose, $D_x\%$, was less than 0.55% of the maximum dose for electron beam of energies 4 MeV - 8 MeV, 0.84% for 10 MeV and

1.44% for electron beam of energy 12 MeV. These percentages are within the tolerance limits of 1% for electron beam energy 4 MeV, and 4% for electron beam energy 20 MeV (Podgorsak, 2003). Table 3 shows that the most probable energy $E_{p,0}$ is higher than the mean energy \bar{E}_0 due to the spread of the electron beam spectrum. The tolerance limit between calculated most probable energy and nominal energy is $\pm 5\%$ (Chosdu, et al., 1995). Thus, the calculated most probable energies are in agreement with the tolerance limit except electron beam of energy 4 MeV and applicator of sizes $14 \times 14 \text{ cm}^2$ and $20 \times 20 \text{ cm}^2$ which exceeded the tolerance limit. Furthermore, the values of dose gradient G for all electron beam energies agree with the lower limit of 2.3.

The relation between mean energy \bar{E}_0 and R_{50} is linear and is in agreement with the theoretical results of Monte Carlo calculations (HPA, 1975).

The values of beam flatness and symmetry were calculated according to International Electrotechnical Commission (IEC) (IEC, 1997). The tolerance limits of flatness and symmetry are $\pm 3\%$ and $\pm 2\%$, respectively. It is noticeable that the values of flatness decrease as applicator size increases which means that the values of flatness are field size dependent. The highest value of flatness was 2.94% for electron beam energy 4 MeV and applicator size $14 \times 14 \text{ cm}^2$, whereas the lowest value was 1.10% for electron beam energy 10 MeV and applicator size $20 \times 20 \text{ cm}^2$. The values of flatness meet the tolerance limit of $\pm 3\%$. The values of symmetry range from 0.03% to 1.93%. This means that the values of symmetry for all energies and two applicators of size $14 \times 14 \text{ cm}^2$ and $20 \times 20 \text{ cm}^2$ are well in agreement with the manufacturer's specifications and IEC.

Table 4 also shows that the penumbra width is an electron energy and field size dependent. The penumbra width is a decreasing function of electron beam energy and field size. The maximum recorded value of the penumbra was 1.30 cm for electron beam energy 4 MeV and applicator size $14 \times 14 \text{ cm}^2$, while the minimum recorded value of the penumbra was 0.96 cm for electron beam energy 12 MeV and applicator size $20 \times 20 \text{ cm}^2$.

The results of applicator factor show that the applicator factor is increased as the applicator size increased for energies 4 and 6 MeV, whereas for energies 8, 10 and 12 MeV is decreased as the applicator size increased. The results are in agreement with Varian TrueBeam and Elekta Versa HD studies (Glide et al., 2013; Narayanasamy et al., 2016).

CONCLUSION

In this work, the electron beams commissioning of an Elekta Synergy platform linear accelerator were presented and analyzed. The results show that the penetrative quality for all electron beam energies were within the tolerance limit of $\pm 1 \text{ mm}$. Bremsstrahlung contamination obtained from measured (PDD) was less than 1.5% for electron beam of nominal energy of 12 MeV which is within the tolerance limits. Values of dose gradient G meet the lower limit of 2.3. The relation between the mean energy \bar{E}_0 and R_{50} is linear, and the percentage error between the most probable energy $E_{p,0}$ and nominal energy fall within the $\pm 5\%$ limit. Beam flatness and beam symmetry, which characterized the beam profiles, meet the IEC 60731 tolerance. The penumbra width is a decreasing function of electron beam energy. The maximum value of the penumbra recorded was 1.30 cm for 4 MeV, whereas the minimum value was 0.96 cm. for 12 MeV. Finally, it is concluded that the measured data of all electron beam energies were found to be within permissible limits. Therefore, all energies of the electron beam can safely be used for clinical purposes.

Duality of interest: The authors declare that they have no duality of interest associated with this manuscript.

Author contributions: The first and the third authors did the measurements and collected all nec-

essary data needed. All authors were involved in the discussion of the results. First author wrote the paper with contributions from the second and third coauthors.

Funding: This work is not funded.

REFERENCES

- Acquah, G. F., & Schiestl, B. (2014). Quality assurance and performance evaluation of an Elekta linear accelerator: results from over a year QA experience in Ghana. *IJSBAR*, 14, 356-363.
- Arun Kumar, T., Supe, S. S., Ravikumar, M., Sathiyar, S., & Ganesh, M. (2010). Electron beam characteristics at extended source-to-surface distances for irregular cut-outs. *Journal of Medical Physics/Association of Medical Physicists of India*, 35(4), 207.
- Brahme, A., & Svensson, H. (1976). Specification of electron beam quality from the central-axis depth absorbed-dose distribution. *Medical physics*, 3(2), 95-102.
- Chosdu, R., Hilmy, N., Tobing, R., Kicky, L. T. K., Razzak, M., Kovacs, A., & Miller, A. (1995). Dosimetry measurements during the commissioning of the GJ-2 electron accelerator. *Radiation Physics and Chemistry*, 46(4-6), 1175-1179.
- Elekta customer acceptance test. (2007). Elekta Oncology Systems Ltd. Crawley: Document number 4513 370 1870 08
- Gerbi, B. J. (2006). Clinical Applications of High-Energy Electrons. In Levitt, S. H., Purdy, J. A. editors. *Technical Basis of Radiation Therapy. Medical Radiology (Radiation Oncology)*, Berlin, Springer.
- Gerbi, B. J., Antolak, J. A., Deibel, F. C., Followill, D. S., Herman, M. G., Higgins, P. D., ... & Khan, F. M. (2009). Recommendations for clinical electron beam dosimetry: supplement to the recommendations of Task Group 25. *Medical physics*, 36(7), 3239-3279.
- Glide-Hurst, C., Bellon, M., Foster, R., Altunbas, C., Speiser, M., Altman, M., ... & Solberg, T. (2013). Commissioning of the Varian TrueBeam linear accelerator: a multi-institutional study. *Medical physics*, 40 (3), 031719.
- Hospital Physicist Association., (1975). A practical guide to selection dosimetry below 5 MeV for Radiotherapy purposes. London: HPA Report No. 13
- International Atomic Energy Agency (IAEA). (1987). Absorbed Dose Determination in Photon and Electron Beams: An International Code of Practice for Dosimetry. Technical Report Series No. 277, Vienna, Austria
- International Atomic Energy Agency (IAEA). (2000). Absorbed Dose Determination in External Beam Radiotherapy: An International Code of Practice for Dosimetry Based on Standards of Absorbed Dose to Water. Technical Report Series No. 398, Vienna, Austria
- International Commission on Radiation Units and Measurements (ICRU). (1993). Prescribing, recording, and reporting photon beam therapy. ICRU report No. 50, Washington, DC, USA

- International Electrotechnical Commission. (1984). Report 35-I and 35-II, Medical electrical equipment, Medical Electron Accelerator, Section IV: Functional performance characteristics and report, Geneva, Switzerland
- International Electrotechnical Commission. (1997). Medical Electrical Equipment: Dosimeters with ionization chambers as used in radiotherapy standard. IEC-60731, Geneva, Switzerland
- International Electrotechnical Commission. (2007). Medical electrical equipment, Medical Electron Accelerators: Functional performance characteristics. IEC-60976, Geneva, Switzerland
- Jamshidi, A., Kuchnir, F. T., & Reft, C. S. (1987). Characteristic parameters of 6–22 MeV electron beams from a 25-MeV linear accelerator. *Medical physics*, 14(2), 282-288.
- Khan, F. M. (2010). *Physics of Radiation Therapy*. 4th edition. Philadelphia, Lippincott Williams & Wilkins, USA.
- Khan, F. M. (1991). Clinical electron-beam dosimetry. Report of AAPM Radiation Therapy Committee Task Group 25. *Med. Phys.*, 18, 73-109.
- Kirby, T. H., Gastorf, R. J., Hanson, W. F., Berkley, L. W., Gagnon, W. F., Hazle, J. D., & Shalek, R. J. (1985). Electron beam central axis depth dose measurements. *Medical physics*, 12(3), 357-361.
- Kutcher, G. J., Coia, L., Gillin, M., Hanson, W. F., Leibel, S., Morton, R. J., ... & Wingfield, L. (1994). Comprehensive QA for radiation oncology: report of AAPM radiation therapy committee task group 40. *Medical Physics-Lancaster PA*-, 21, 581-581.
- Narayanasamy, G., Saenz, D., Cruz, W., Ha, C. S., Papanikolaou, N., & Stathakis, S. (2016). Commissioning an Elekta Versa HD linear accelerator. *Journal of applied clinical medical physics*, 17(1), 179-191.
- Podgorsak, E. B. (2003). Review of radiation oncology physics: a handbook for teachers and students. *Vienna, Austria: IAE Agency*, 19, 133.
- Sahool, S. K., Rath, A. K., Mukharjee, R. N., & Mallick, B. (2012). Commissioning of a Modern LINAC for Clinical Treatment and Material Research. *International Journal of Trends in Interdisciplinary Studies*, 1(10).
- Varatharaj C, Shwetha B, Rekha Reddy B, Ravikumar M, S. Sathiyar, Ganesh K. M. (2016). Physical characteristics of photon and electron beams from a radiotherapy accelerator. *International Journal of Medical Research and Review Res Rev* .4 (7), 1178- 1188.